


Lab name: SRI Instruments  
 Client: SRI Final test  
 Client ID: N11811  
 Analysis date: 03/08/2022 09:22:53  
 Method: Heated Inj 200C  
 Description: SameDataAsCh1 by area%  
 Column: 30MXT500  
 Carrier: H2fromBIING  
 Integration: Peak sens=95.0 Base sens=60.0 Min area= 10.00 Standard= 4.000 Sample=100.000 Tangents=off  
 Data file: 333calMXT523.CHR ()  
 Sample: 167ng/l calibration

Temperature program:  

Init temp	Hold	Ramp	Final temp
140.00	0.000	20.000	200.00
200.00	0.000	5.000	225.00
80.00	0.000	30.000	140.00

Events:  

Time	Event
0.000	ZERO
0.000	SOUND
2.000	INTEG IMMEDIATE

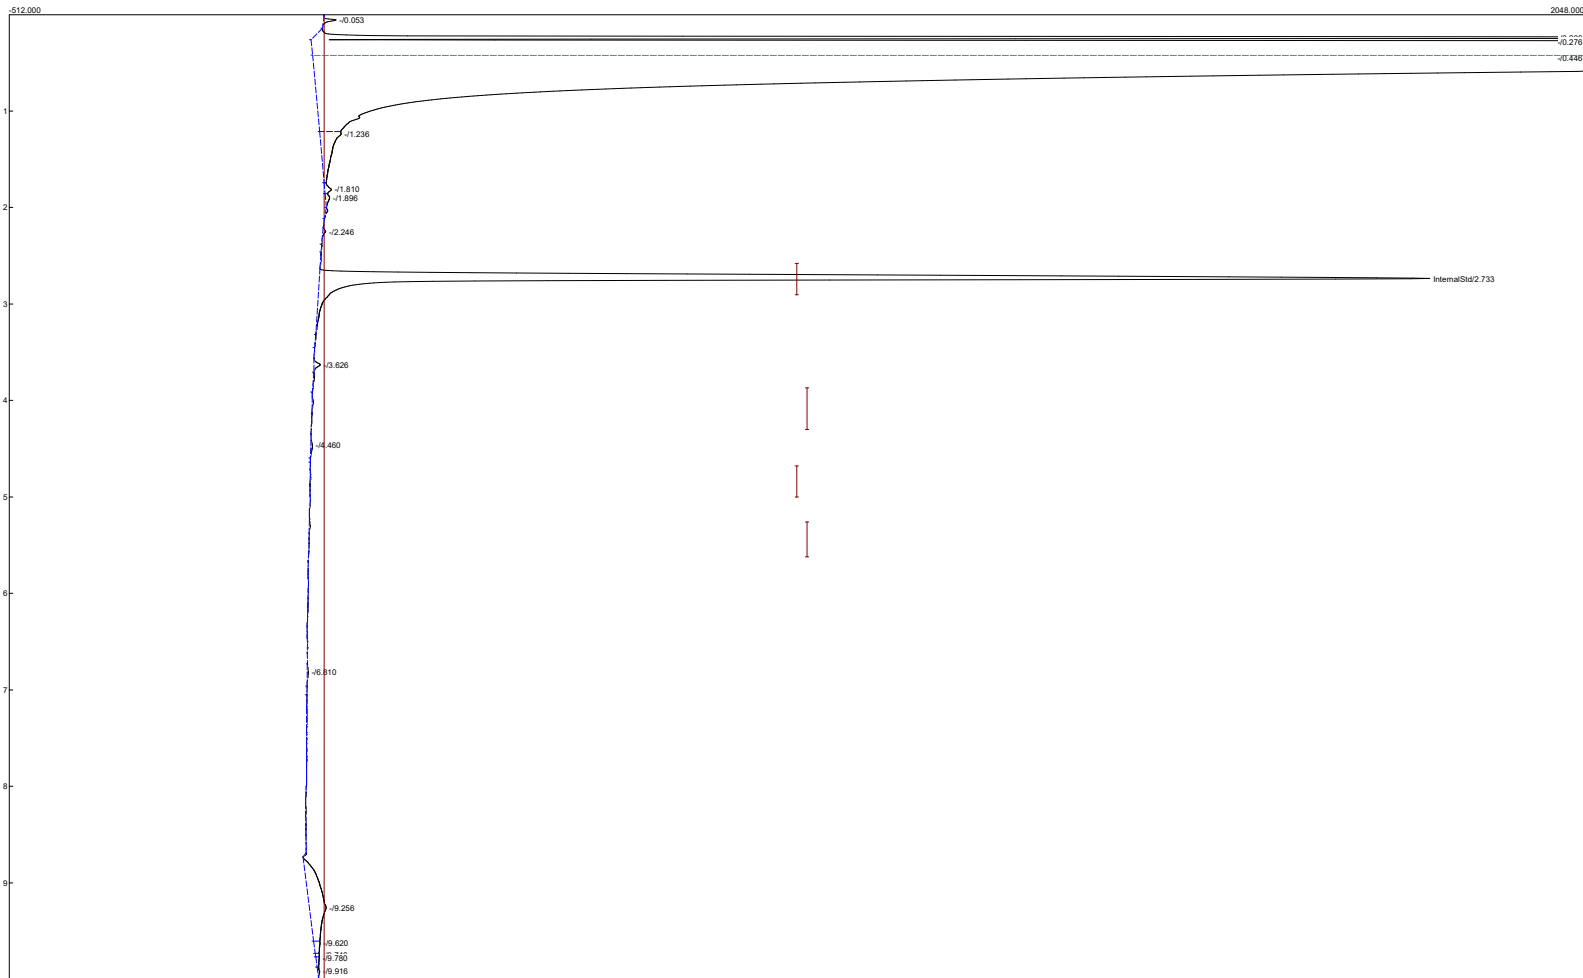

Component	Retention	Area	Internal	Norm area %Units
InternalStd	2.733	6310.6434	100.0000	100.0000
CBD	0.000	0.0000	0.0000	0.0000 %
Δ9THC	0.000	0.0000	0.0000	0.0000 %
CBN	0.000	0.0000	0.0000	0.0000 %
		6310.6434	100.0000	100.0000