



Customer: **Allied Central Marketing, LLC**  
 Customer Sample ID: **KifCure Full Spec Organic 10-6-2020**  
 Laboratory Number: **20J0134-01**



## Cannabinoid Profile


Extraction Technician: DF  
 Analytical Chemist: CB

Extraction Date(s)	Analysis Date(s)
10/7/2020	10/7/2020

Cannabinoids (HPLC)		Results	
	LOD (mg/g)	%	mg/g
Cannabidiol (CBD)		87.21	872
delta 9-Tetrahydrocannabinol (THC)		3.00	30.0
Cannabidiol (CBD)		0.15	1.50
Cannabidiolic Acid (CBD-A)	<0.40		
Cannabigerolic Acid (CBG-A)	<0.40		
Cannabigerol (CBG)		0.99	9.86
Tetrahydrocannabivarin (THCV)	<0.40		
Cannabinol (CBN)		0.24	2.38
delta 8-Tetrahydrocannabinol	<0.40		
Cannabichromene (CBC)	<0.40		
delta-9-Tetrahydrocannabinolic Acid (THC-A)	<0.40		
Cannabinoids Total		%	mg/g
Max Active THC		3.00	30.00
Max Active CBD		87.20	872.00
T.Active Cannabinoids		91.40	914.00
Total Cannabinoids		91.60	916.00

Following USDA guidelines on uncertainty, Altitude Consulting's uncertainty are calculated for CBDa and CBD at +/- 4%. The uncertainty for THCa and THC are +/- 5%. This implies the range for a 10% value of CBD to be 9.6-10.4%. The uncertainty range for a 0.30% value of THC would be 0.28-0.32%. The measurement uncertainty is calculated using a coverage factor of 2.

### Cannabinoid (mg/g)

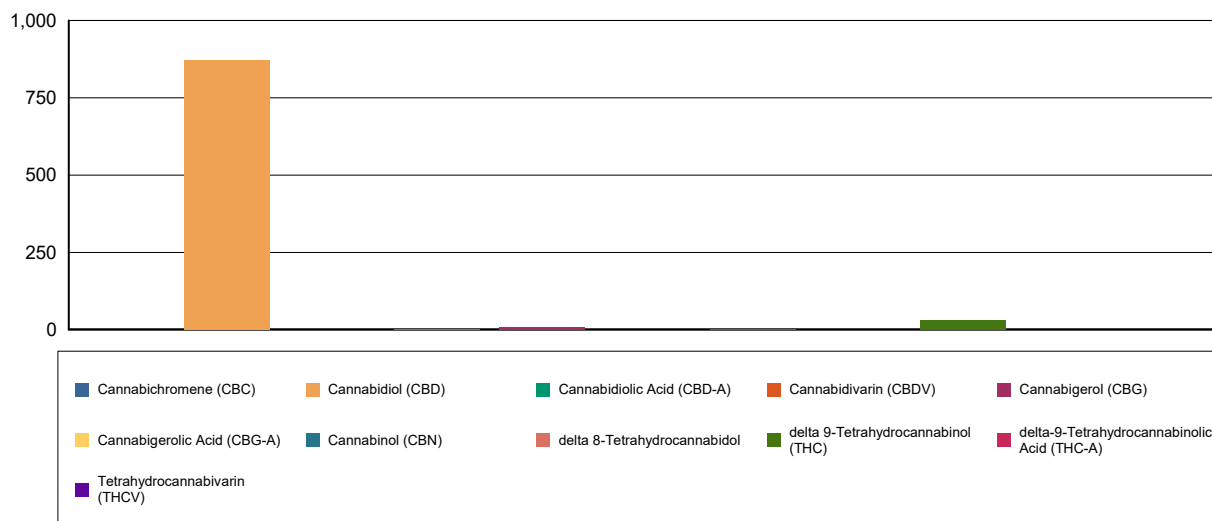

Reporting Limits will vary based on sample extraction weight used for the analysis.

Altitude Consulting, LLC utilizes NIST traceable Reference Standards and Certified Reference Material to calibrate analytical instruments along with proven analytical methods. The methods are applied in the most ethical manner following good laboratory practice guidelines. The results of this report are based solely on the sample submitted and cannot be reproduced.



**Customer:** Allied Central Marketing, LLC  
**Customer Sample ID:** KifCure Full Spec Organic 10-6-2020  
**Laboratory Number:** 20J0134-01



## Residual Solvents Profile

Extraction Technician: DF  
 Analytical Chemist: CB

Extraction Date(s)	Analysis Date(s)
10/7/2020	10/7/2020

Residual Solvents	Results	Calibration Range
	ug/g	
Propane	<96.0	100 - 2000
Isobutane	<96.0	100 - 2000
Methanol	<96.0	100 - 2000
Butane	<96.0	100 - 2000
Isopropanol	<96.0	100 - 2000
Ethanol	<96.0	100 - 2000
2-Methyl Butane	<96.0	100 - 2000
Acetonitrile	<96.0	100 - 2000
Acetone	<96.0	100 - 2000
n-Pentane	<96.0	100 - 2000
n-Hexane	<48.0	50 - 2000
Tetrahydrofuran	<96.0	100 - 2000
Benzene	<0.960	1.0 - 50
n-Heptane	<96.0	100 - 2000
Toluene	<96.0	100 - 2000
Ethylbenzene	<96.0	100 - 2000
m+p Xylene	<96.0	100 - 2000
o-Xylene	<96.0	100 - 2000

Reporting Limits will vary based on sample extraction weight used for the analysis.

Altitude Consulting, LLC utilizes NIST traceable Reference Standards and Certified Reference Material to calibrate analytical instruments along with proven analytical methods. The methods are applied in the most ethical manner following good laboratory practice guidelines. The results of this report are based solely on the sample submitted and cannot be reproduced.