


Lab name: SRI Instruments
 Client: SRI Final test
 Client ID: N111811
 Analysis date: 03/08/2022 09:09:00
 Method: Heated Inj 200C
 Description: SameDataAsCh1 by area%
 Column: 30MXT500
 Carrier: H2fromBIING
 Integration: Peak sens=95.0 Base sens=60.0 Min area= 10.00 Standard= 4.000 Sample=100.000 Tangents=off
 Data file: 333calMXT522.CHR ()
 Sample: 167ng/l calibration

Temperature program:

Init temp	Hold	Ramp	Final temp
140.00	0.000	20.000	200.00
200.00	0.000	5.000	225.00
80.00	0.000	30.000	140.00

Events:

Time	Event
0.000	ZERO
0.000	SOUND
2.000	INTEG IMMEDIATE

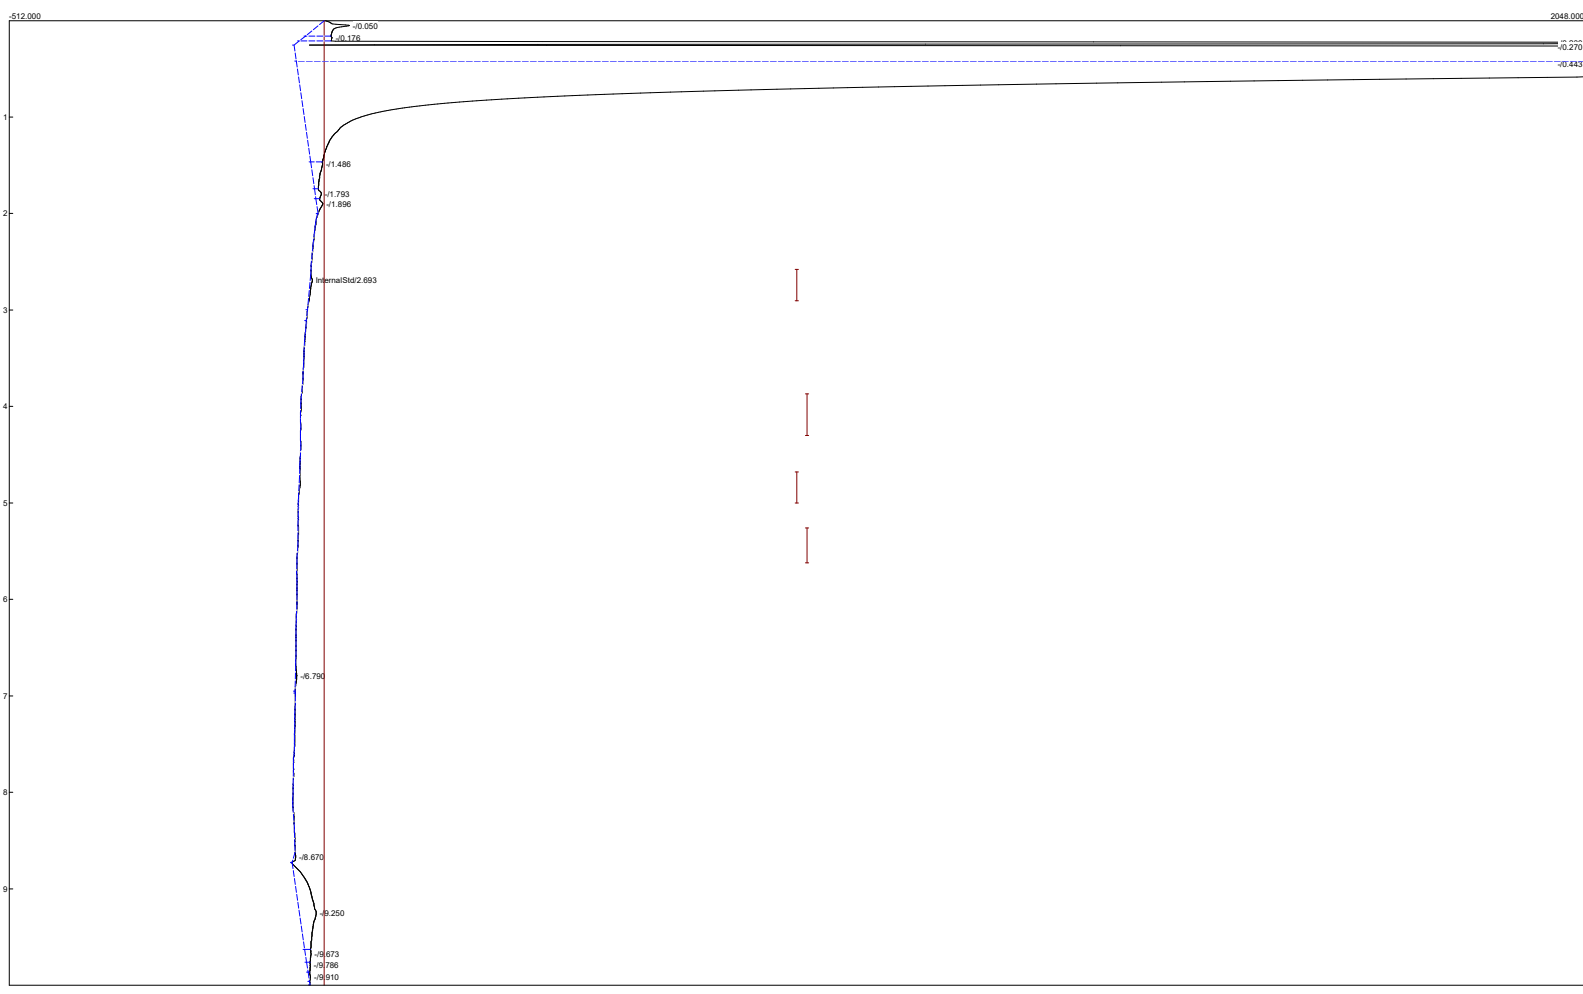

Component	Retention	Area	Internal	Norm area %Units
InternalStd	2.693	33.7157	100.0000	100.0000
CBD	0.000	0.0000	0.0000	0.0000 %
Δ9THC	0.000	0.0000	0.0000	0.0000 %
CBN	0.000	0.0000	0.0000	0.0000 %
		33.7157	100.0000	100.0000